

Stopping Muon Detector (SMD)

Manual for UBC Physics 531 and GRIDS-TSI

Original Author: Matthew Stukel (TRIUMF)
REVISED: 2018/8/01 BY DOUG BRYMAN (DOUG@TRIUMF.CA)

Table of Contents

INTRODUCTION	3
DETECTOR DESIGN.....	3
DESCRIPTION OF ANALYSIS PROGRAM	8
OPERATION	12
STARTING A SINGLE RUN WITH NO TIME LIMIT	13
STARTING MULTIPLE RUNS WITH TIME LIMIT	13
RUNNING AN ANALYSIS LIVE.....	14
RUNNING AN ANALYSIS ON A PREVIOUS RUN	14
TURNING OFF THE DETECTOR	16
PERFORMING YOUR OWN MEASUREMENTS AND ANALYSIS.....	18
ON-LINE SOFTWARE/ANALYSIS.....	18
OUTPUT DATA TEXT FILES.....	18
PROPOSE AND PERFORM MEASUREMENTS.....	19
APPENDIX 1: MOVING THE DETECTOR.....	21
Opening A TRIUMF Network Link.....	22
APPENDIX 2: On-line ANALYSIS PROGRAM HELP	23
INTRODUCTION TO THE ANALYSIS PROGRAM CODE.....	23
ADDITIONAL ANALYSIS SCRIPT.....	23
APPENDIX 3: Signal and HV Cabling.....	29
ACKNOWLEDGMENTS.....	30
REFERENCES.....	30

Introduction

This setup was originally designed to study the effect of low energy muons which can cause single event upsets in electronic devices such as SRAM memories. The particular muons of interest are below 10 MeV (with a range in silicon of a few mm) and may cause upsets when the muon deposits most of its energy. There are older measurements of the rate of low energy muons at surface level but these measurements differ by up to an order of magnitude and did not positively identify the particles as muons.

This manual discusses the design and operation of a detector capable of identifying low energy stopping muons and their decay products. The detector can be used to measure the energy and rate of the stopping muons. The detector is portable and large in volume in order for measurements to be made under various conditions (i.e. altitude, latitude and location within TRIUMF). Due to the size of the detector it is also able to get appropriate statistics for the muon lifetime and rate in under 12 hours. It can also distinguish between muons that stop in the detector and muons that pass through. The detector was built at TRIUMF Canada's National Particle and Nuclear Physics Laboratory. The initial design study for this detector was funded by Cisco Systems in San Jose, CA. For an example of the use of the detector for Soft Error studies see ref^[1].

For the Physics 531/GRIDS-TSI lab, the detector can be configured in various ways to make measurements which relate to the scintillator and PMT properties and performance such as time and energy resolutions as well as properties of muons such as the decay energy spectrum and lifetime. The section below Performing your Own Measurements and Analysis describes some example measurements you can make with this setup.

Please read the entire manual before operation of the detector.

Detector Design

The Stopping Muon Detector (SMD) consists of four 10cm x 10cm x 100cm plastic scintillator rectangles. The plastic material is Bicron-400 (BC-400). As a muon passes through each scintillator visible wavelength photons are emitted. The light output of the scintillator is proportional to the energy lost by the particle that traverses the detector. See Fig 1.

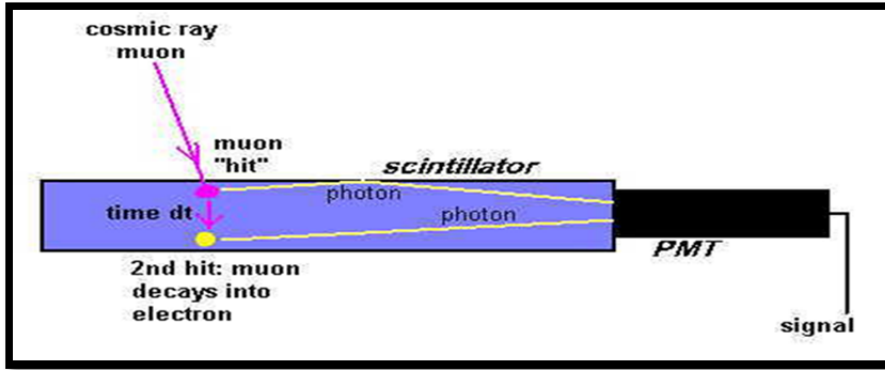


FIG 1: Schematic diagram of a muon stopping and decaying in a plastic scintillator.^[12] In the lab configuration, the scintillator bars are viewed at both ends by PMTs.

The scintillation photons are transmitted directly and through total internal reflection to a light guide and to a photomultiplier tube (PMT) which converts the signal to a small current, and amplifies the signal producing a measurable current. Each scintillator bar has a Philips XP2262 PMT at each end (making for a total of 8). PMT's consist of a photocathode and a series of powered dynodes in an evacuated glass structure. When the photons from the scintillator strike the photo-cathode, electrons are emitted with some probability (the quantum efficiency, typically 15-30%). The electrons are accelerated towards a series of additional electrodes called dynodes. This cascading effect creates 10^5 - 10^7 electrons for each photo-electron emitted. See Fig 2.^[6]

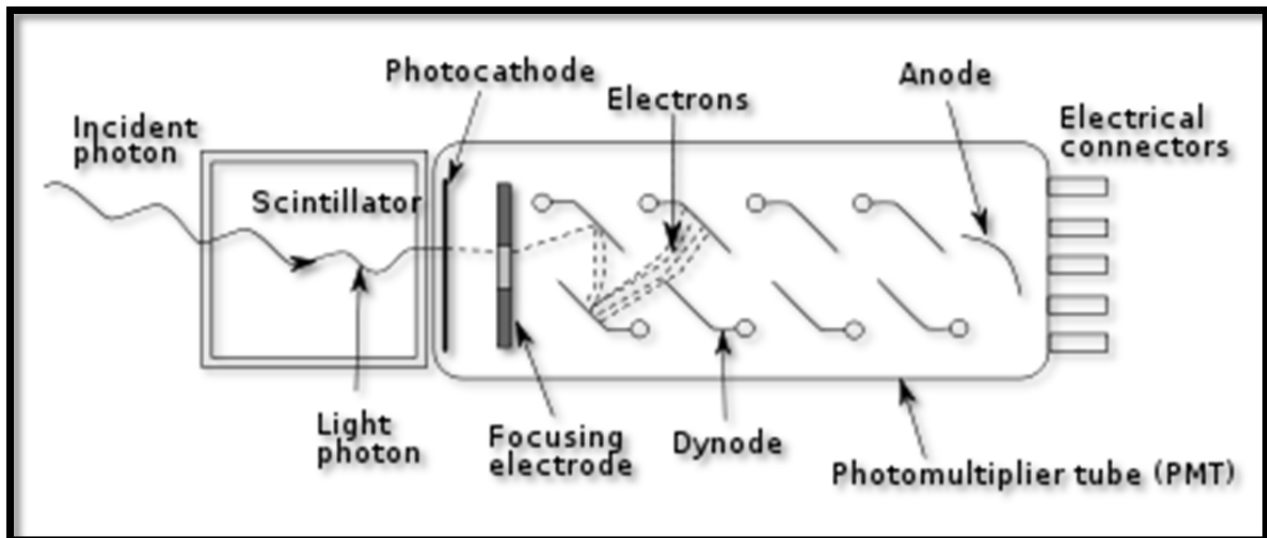


FIG 2: Schematic diagram of a gamma ray (e.g. an X-ray) producing light in a scintillator which impinges on the PMT.^[2]

The PMT's are powered by a CAEN V6533, 6 Channel VME^[3] Programmable HV Power Supply. The board is available with either positive or negative output polarity. The HV outputs

are delivered through Safe High Voltage (SHV) connectors. Each PMT has been set at a voltage to produce about the same pulse height for passing through muons. The scintillators are labeled 1-4, with light guides labeled a and b on each end. See table 1 and Appendix 3. There are only 6 HV channels for 8 PMTs so one set of PMT's shares voltages; PMT 1b and 2a share HV output 4 and PMT 4a is connected to an external Fluke (manufacturer) power supply.

HV Output	Voltage (V)
0	1693
1	1644
2	1680
3	1550
4	1663
5	1584
Fluke	1650

TABLE 1: High Voltage Settings

In addition, to the HV Power supply the PMT's last dynode outputs are connected to CAEN V1720 flash ADCs. See Appendix 1. The V1720 ^[4] houses 8 channels of 12 bit 250 MS/s Flash ADC Waveform Digitizer. In this module the analog to digital conversion occurs as close as possible to the detector. The operation of the digitizer is similar to an oscilloscope; when a trigger occurs, a certain number of samples are saved into one memory buffer. An algorithm (in the V1720) will continuously calculate the baseline of the input signal by averaging the samples over a moving window. The input signal is compared against the value of the trigger threshold and the trigger fires as soon as it is crossed by the signal – thus, the ADC is self-triggered by any observed pulse. The trigger enables the event building and the event data is saved into a memory buffer. The control software automatically optimizes both the number of events inside the buffer and the number of total buffers in the memory ^[15]. The integral of the pulse charge corresponds to the energy of the incident particle; calibration is required before actual energy units can be assigned. In addition, a time stamp of the trigger is recorded. Fig. 3 illustrates a single pulse and its parameters. (The specific detector parameters can be seen in Table 2)

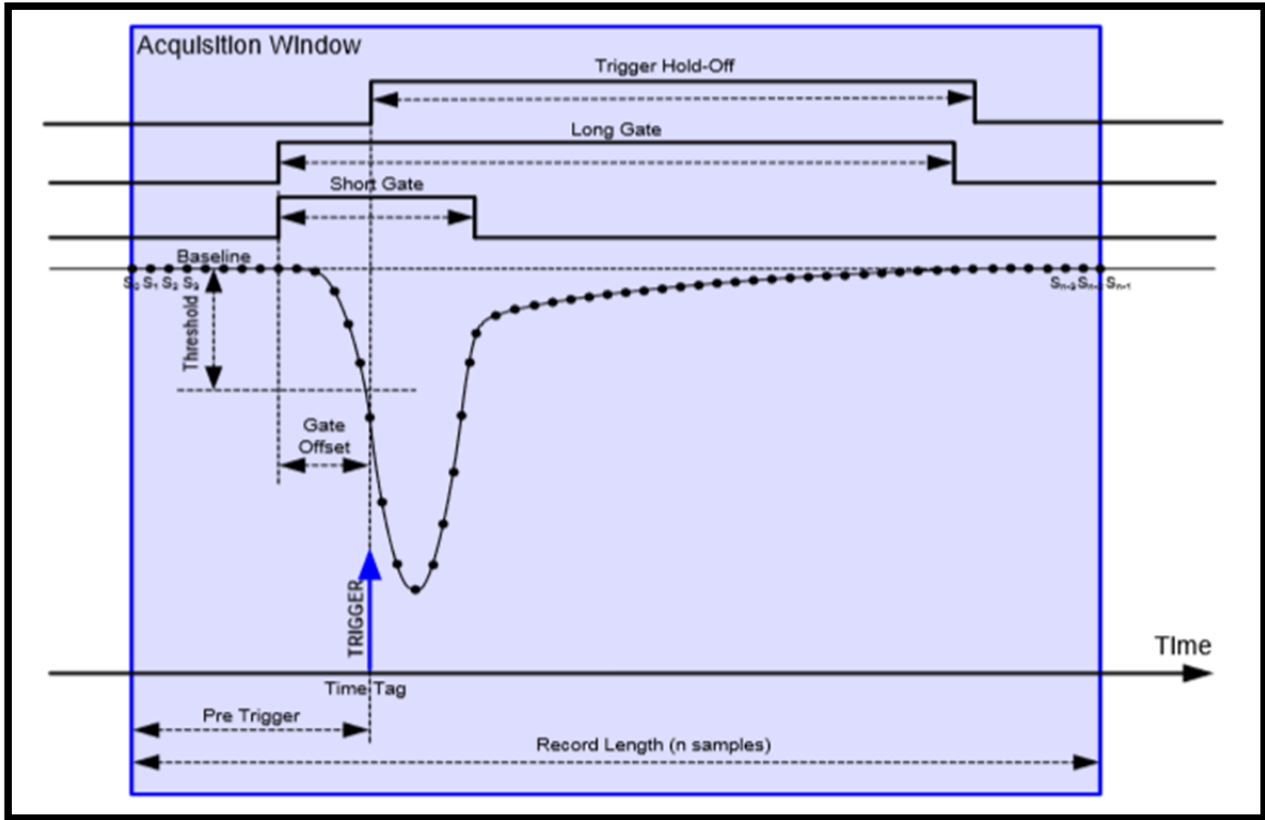


FIG 3: Diagram illustrating the pulse parameters. The trigger fires as soon as the signal crosses the threshold. ^[15]

Parameter	Value
Trigger Hold-Off	80 ns
Long Gate	200 ns
Short Gate	40 ns
Threshold	100
Pre Trigger	12 ns

TABLE 2: Details the parameters of the V1720.

Both the V1720 and the V6533 are controlled by the master module, CAEN V1718 ^[5]. The module is operated through a USB port to a Laptop. The V1718 provides all the addressing and data transfer. The V1720, V6533 and V1718 are all contained in a standard VME crate. The laptop uses the MIDAS (Maximum Integrated Data Acquisition System) developed at TRIUMF. MIDAS provides the frontend template for acquiring hardware information, data transfer, full run control and web interface for experimental control. A tailored analysis program (using some of the MIDAS framework as a backbone) was developed for demonstration as discussed below. The analysis program uses coincidence gating to detect stopping muons and project their spectrum. Custom analysis of the data can also be done as described below.

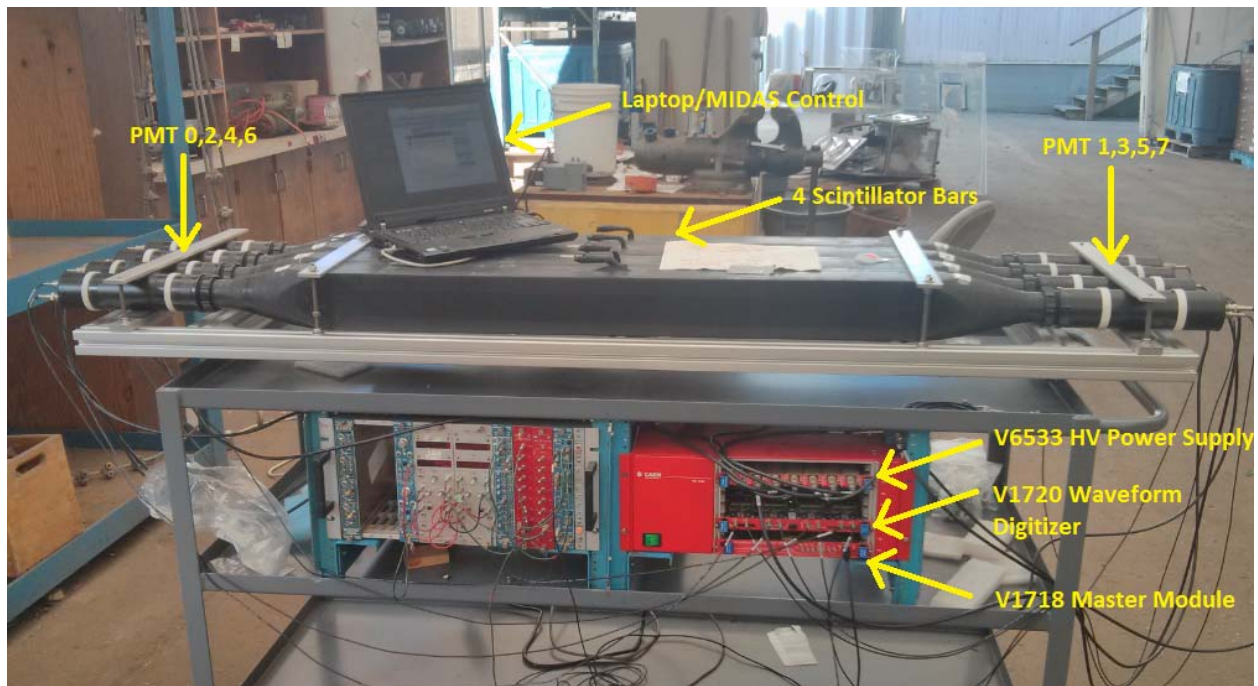


FIG 4: Shows the detector completely assembled with the control laptop. PMTs 0, 2, 4, and 6 (1,3,5,7) are associated with light guides 1a, 2a, 3a, and 4a (1b, 2b, 3b, and 4b).

One of the unique things about this detector is it's customizable configuration. There have been three main setups; 1) 4x1 horizontally 2) 2x2 setup 3) 4x1 configuration.

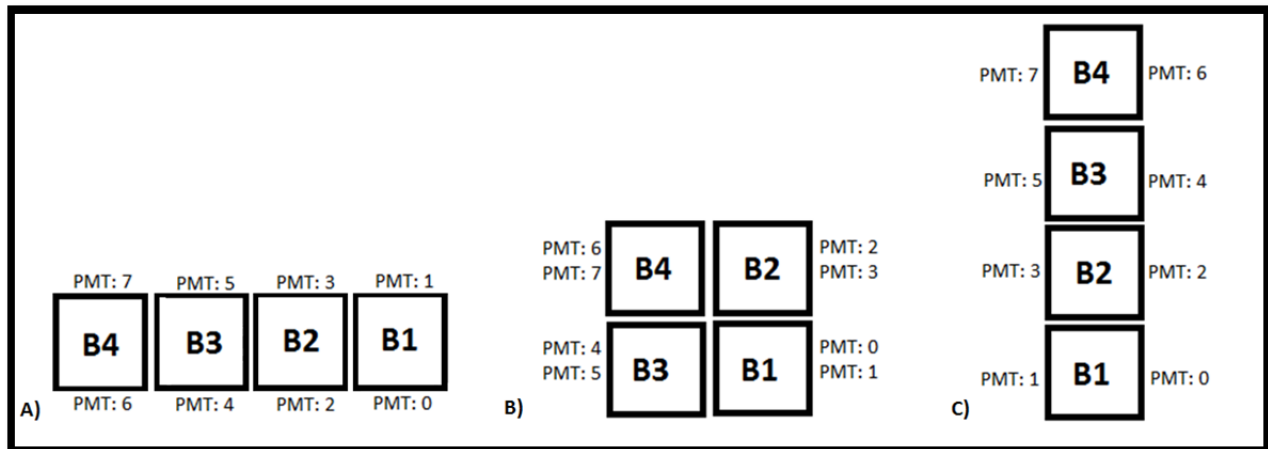


FIG 5: Some possible configurations of the SMD; A) 4x1 horizontally B) 2x2 setup C) 4x1 vertically. Before re-configuring the setup, turn high voltages off.

Description of Analysis Program

The SMD detector can be set to take data for a specific amount of time or to be free running. During operation, it will sense all particles (muons being the most abundant) that pass directly through the scintillator as well as the muons that stop to decay. The analysis program is designed to distinguish between these two events. A particle that will pass through will excite the scintillator producing a pulse. The integrated pulse energy of this particle is put in a histogram called the “Passing Through Event Spectrum”. An example of this spectrum is given in Fig 6.

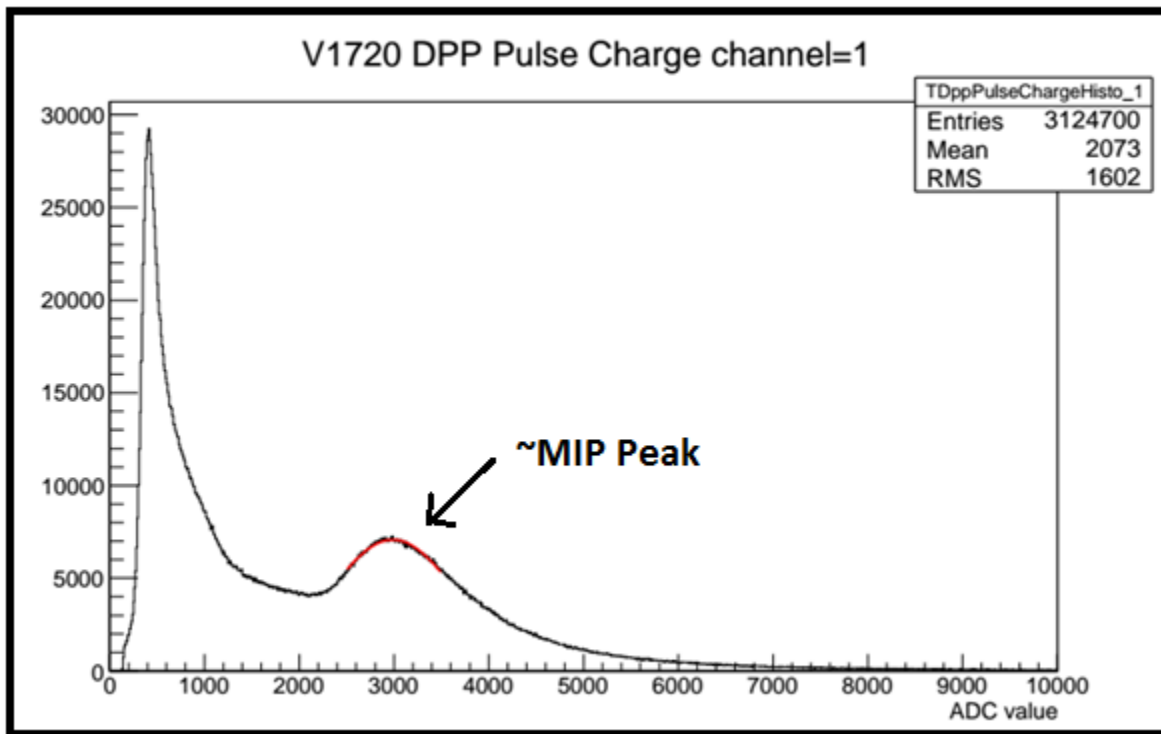


FIG 6: A standard “Passing Through Event Spectrum” of cosmic radiation.

Note that the ADC value is recorded because the energy calibration has not yet been completed. The Minimum Ionizing Particles (MIP) peak corresponds to cosmic muons that don't stop. The peak is roughly at 22 MeV. There is also a chance that muons which have low enough energy to stop in a bar will decay into an electron (See Eq. 4-5) inside the bar. This will produce two pulses in the same bar and may cause coincidences with other bars. See Fig 7 for pulse comparisons. The muon lifetime is 2.2 μ s.

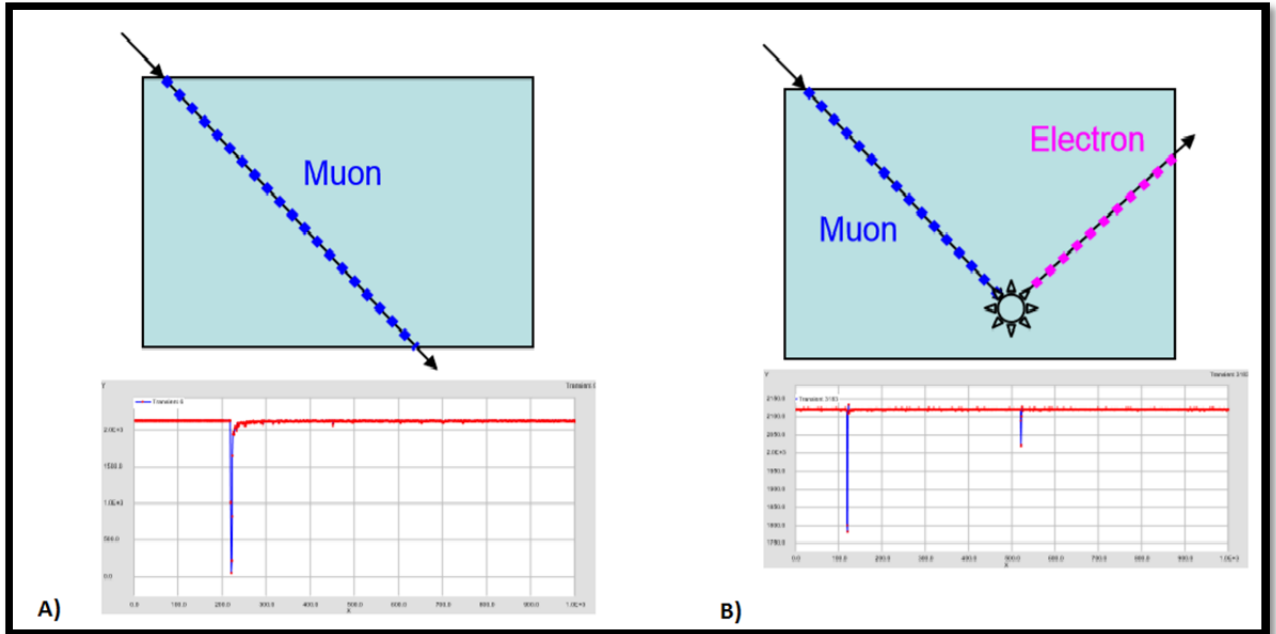


FIG 7: A) A muon (or other particle) that passes through the detector without decaying B) A muon that stops and decays into an electron inside the bar.^[17]

If the time difference between the pulses is less than 20 μs the difference is recorded in the “Time Difference Histogram”. See Fig. 8 for an example. This histograms corresponds to the decay time distribution (which is used to fit the distribution)

$$D(t) = \lambda \exp(-\lambda t) + B \quad (1)$$

If the parameters of the fit indicate a lifetime of $\sim 2.2 \mu\text{s}$ the particle can be identified as a muon. (Cosmic rays may consist of both positive and negative muons which have slightly different lifetimes when stopped in plastic scintillator. Do you know why?)

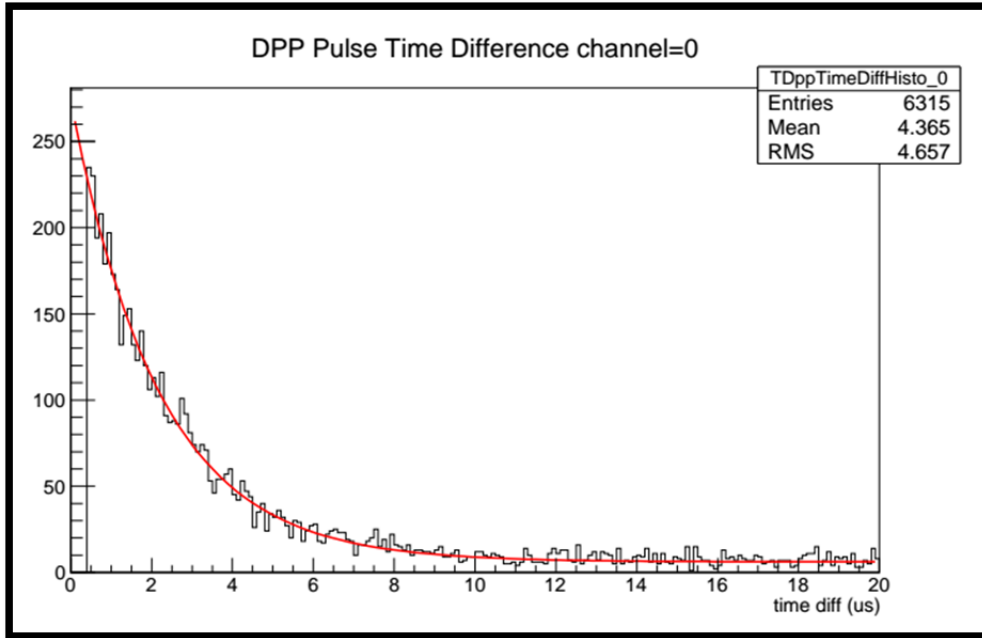


FIG 8: A standard muon decay time distribution

Once identified as a muon (2 pulses found) the energy spectrum of the muon which decayed and its decaying electron are recorded. See Fig 9-10 for the muon and electron energy spectrums respectively.

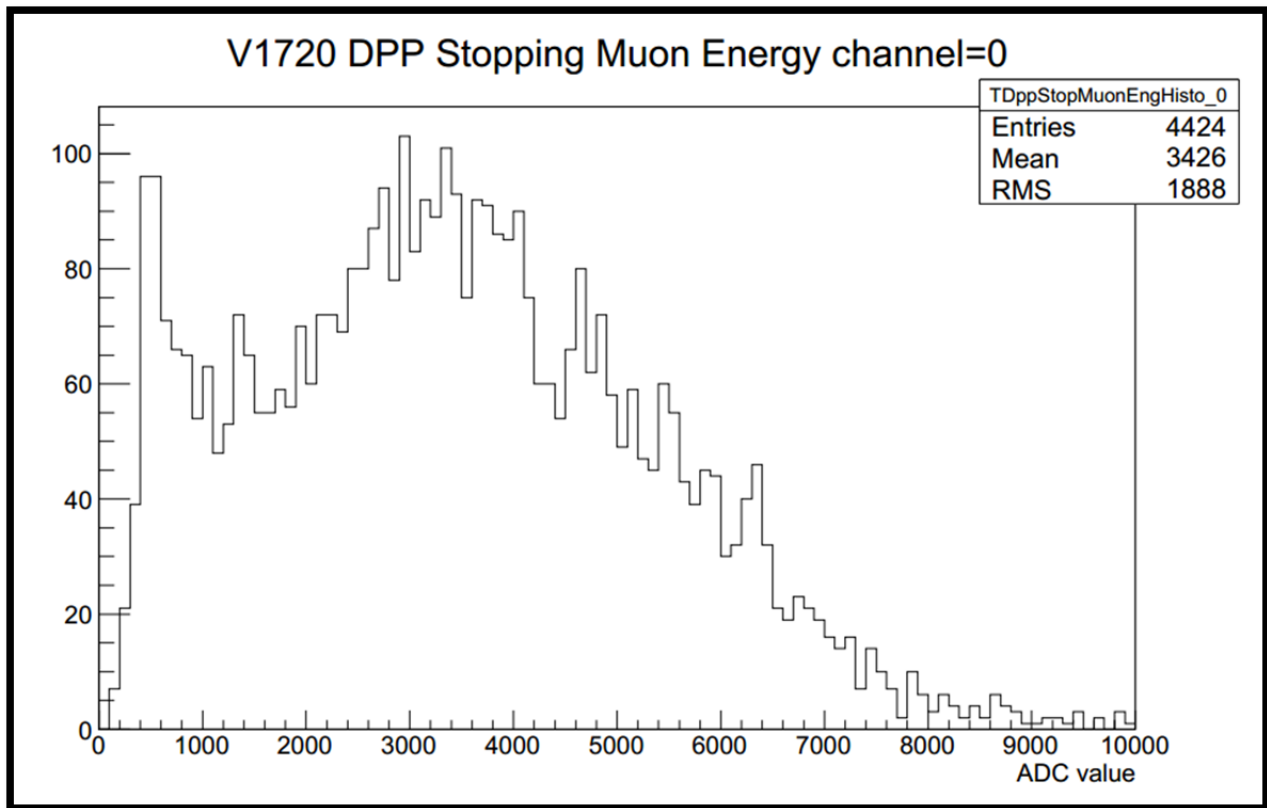


FIG 9: Standard Cosmic Stopping Muon Energy Spectrum

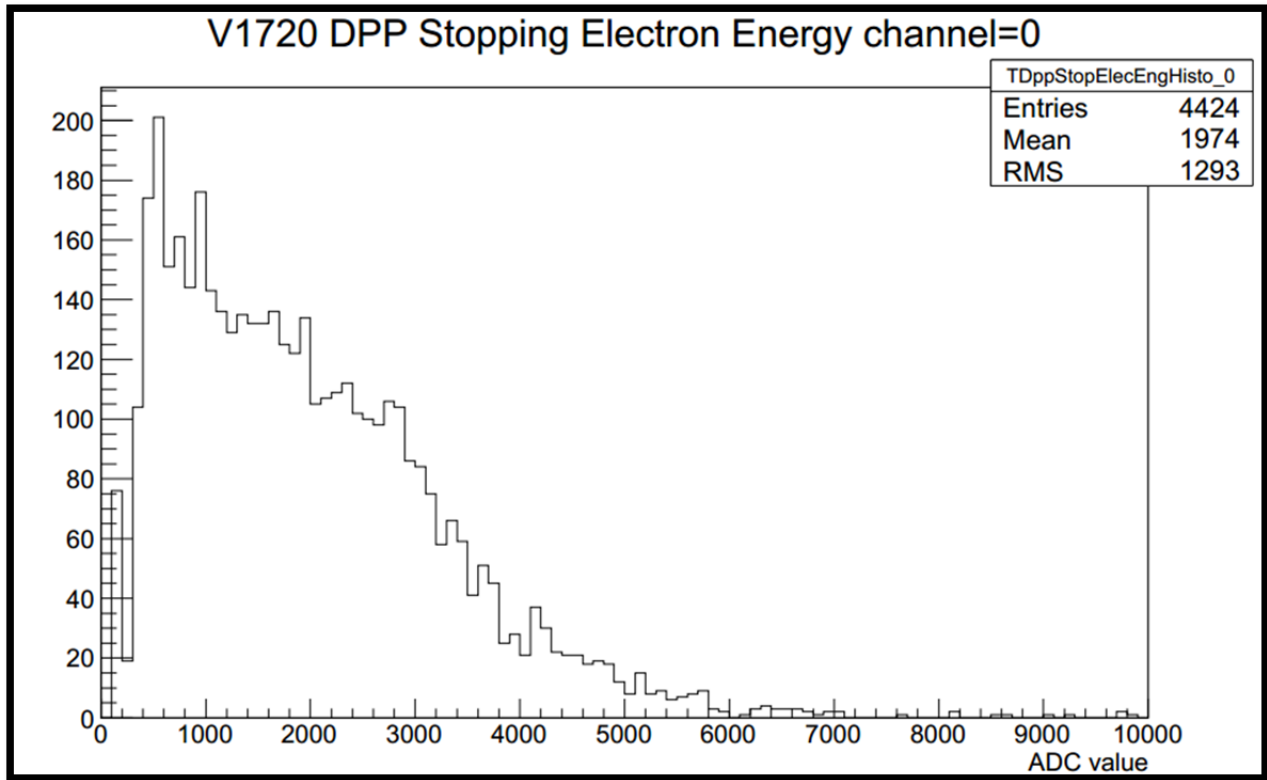


FIG 10: Decaying Electron Energy Spectrum

The above analysis is performed live, separately on each of the PMT's. In the end, this produces eight histograms for the Passing Through Event Spectrum, The Decay Time Distribution, The Stopping Muon Energy Spectrum and The Decaying Electron Energy Spectrum.

From an average cosmic ray spectrum (i.e. no external sources or shielding) there is an average of ~ 130 muons/sec that pass through while only 16 muons/min stop. The detector is able to distinguish between these events.

There are many other measurements that can be done with this system using the pulse data from the PMTs as discussed below (see "Performing your own Measurements and Analysis").

Operation

There are two main parts to the Stopping Muon Detector. The MIDAS front end and the tailored analysis program. The detector is controlled by the laptop through the front end MIDAS system. Here all aspects of the detector can be changed.

The laptop name is daqlap01.triumf.ca. An account has been setup named daquser which requires a pw which will be supplied.

The daq system is controlled via a web interface: <http://daqlap01.triumf.ca:8081/> which looks as follows:

Run Status

Run 398 Stopped
 Start: Tue Aug 19 10:30:34 2014
 Stop: Wed Aug 20 10:04:11 2014
 Alarms: Off Restart: Yes
 Data dir: /home/midas/online/
 Comment: L2 of the Ariel Building (4x1 arrangement)
 10:20:54 [Logger1,INFO] Program Logger1 on host lpdaq02 stopped

Equipment

Equipment	Status	Events	Events[s]	Data[MB/s]
V6533	(frontend stopped)	41692	0.6	0.000
FEV1720PSD	(frontend stopped)	1.821M	0.0	0.000
BUFLVL	(frontend stopped)	0	0.0	0.000

Logging Channels

Channel	Events	MB written	Compr.	Disk level
#0: run00398.mid.gz	1862358	1111.097	52.3%	70.6 %

Clients

Logger [lpdaq02] mhttpd [lpdaq02]

FIG 11: MIDAS control system

Before starting a run, make sure that the FEV1720PSD and V6533 frontend programs are running. If they are not, go to the programs page and start them

<http://daqlap01.triumf.ca:8081/?cmd=Programs>

The FEV1720PSD program is the program that acquires the data from the digitizer board.

When the frontend programs are running, you can start a run. You can decide whether you actually want to write the data for a particular run. The trigger rate for the V1720 is ~18Hz.

The six PMT high voltage values are set via the ODB tab on the main Status page. Choose “Equipment” and then “V6533”, then “Variables” view, set, or change the HV values (which are normally set to nominal values). Scintillator PMT 4a is controlled by a separate manual Fluke HV power supply. *Consult the lab supervisor before changing the HV.* The nominal HV values are set to put the pass through muon peak at roughly the same adc sum value

Starting A Single Run With No Time Limit

If the detector is completely set up there is an easy way to start a run. This run will only stop when stopped manually.

STEP 1: Open the MIDAS control: This can be done through two links

- ➔ TRIUMF network connected: Type the URL: **daqlap01.triumf.ca:8081**. If the link does not open. See Opening A TRIUMF Network Link.
- ➔ TRIUMF network not connected: Type the URL: **localhost:8081**

STEP 2: Select the **START** button in the red square of the MIDAS control




FIG 12: Start button of MIDAS control

STEP 3: A screen will appear asking for a comment and a run number (Enter a comment if you need to.)

STEP 4: The run will continue until the user manually presses the **STOP** button

Starting Multiple Run's With Time Limit

There is a way to allow multiple runs of a specific time.

STEP 1: On the MIDAS front end control panel select the **SEQUENCER** tab




FIG 13: Sequencer tab on the MIDAS control

STEP 2: Select the **Start Sequence** button

STEP 3: The screen will then give you the option of selecting the number of runs and the time of each run (in seconds). Once satisfied with those parameters select okay.

STEP 4: The run will then run for the given amount of time. After the run is finished the next one will start after a given amount of time. This value can be changed by editing the script

Running an analysis live

It is sometime beneficial to analyse the run as it is taking data. In this way any error or loose cables can be noticed before a lot of time is wasted.

STEP 1: From the laptop open a terminal

STEP 2: Enter: **cd online/src/analyzer**

STEP 3: Enter: **./SmdDisplay.exe**

STEP 4: The analyzer program will then appear and data will start to fill the histograms. The analysis program includes the Passing Through Event Spectrum, The Decay Time Distribution, The Stopping Muon Energy Spectrum, The Decaying Electron Energy Spectrum and the Waveform Spectrum.

STEP 5: The analysis window will continue to update until the run is stopped and all data points are entered.

Running an analysis on a previous run

Previous runs are saved on the laptop and backed up occasionally by Pierre Amaudruz. The files can be viewed by opening a terminal and entering **cd online**. In this folder all the runs can be viewed. Each run will have two associated files. The first one is run00###.mid.gz which contains all the run data. The second is run00###.odb in this file all information (i.e. parameters) are stored in a text file.

STEP 1: From the laptop open a terminal

STEP 2: Enter: **cd online/src/analyzer**

STEP 3: Enter: **./SmdDisplay.exe ~/Data/run00###.mid.gz -s3000000**; This will start the analyzer, it is very similar to the live analysis except we select a specific run and number of events.

```

stukelm@the-truest-of-homies: ~
Processed 576500 events. Analysis rate = 3723.507246 events/seconds.
Processed 577000 events. Analysis rate = 3695.027232 events/seconds.
Processed 577500 events. Analysis rate = 3694.344697 events/seconds.
Processed 578000 events. Analysis rate = 3709.969430 events/seconds.
Processed 578500 events. Analysis rate = 3712.944811 events/seconds.
Processed 579000 events. Analysis rate = 3711.787151 events/seconds.
Processed 579500 events. Analysis rate = 3708.538539 events/seconds.
Processed 580000 events. Analysis rate = 3716.284013 events/seconds.
Processed 580500 events. Analysis rate = 3701.565022 events/seconds.
Processed 581000 events. Analysis rate = 3731.705315 events/seconds.
Processed 581500 events. Analysis rate = 3694.699584 events/seconds.
Processed 582000 events. Analysis rate = 3729.562000 events/seconds.
Processed 582500 events. Analysis rate = 3738.317757 events/seconds.
Processed 583000 events. Analysis rate = 3726.282214 events/seconds.
Processed 583500 events. Analysis rate = 3704.856326 events/seconds.
Processed 584000 events. Analysis rate = 3682.102038 events/seconds.
Processed 584500 events. Analysis rate = 3685.032870 events/seconds.
Processed 585000 events. Analysis rate = 3723.812290 events/seconds.
Processed 585500 events. Analysis rate = 3478.285066 events/seconds.
Processed 586000 events. Analysis rate = 2053.303766 events/seconds.
Processed 586500 events. Analysis rate = 1985.631967 events/seconds.
Processed 587000 events. Analysis rate = 3698.553126 events/seconds.
Processed 587500 events. Analysis rate = 3744.925626 events/seconds.

```

FIG 14: Events being processed

STEP 4: After step 3 is entered the progress of events analysed will scroll down the terminal. If the number of events chosen is more than the total events of the run the analysis window will not appear. So the first time you do step 3 you should select an abnormally high number of events. In this way you can determine the actual number of events.

STEP 5: Once the progress stops the analysis window will appear.

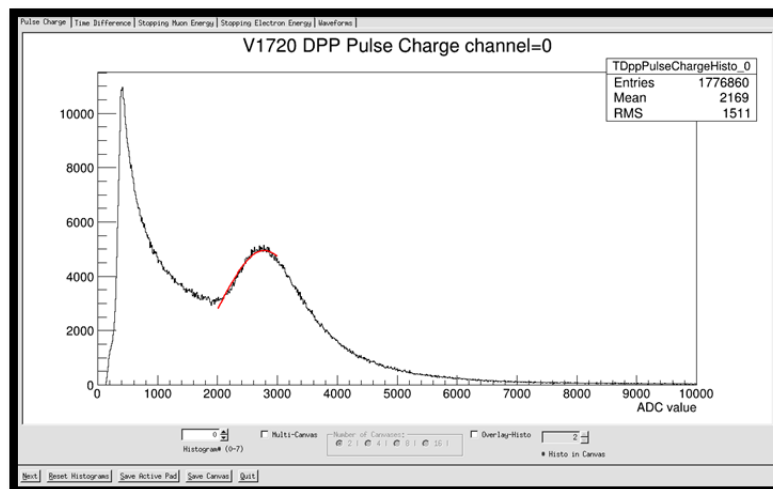


FIG 15: General Analysis Window

STEP 7: The analysis window allows you to save the canvases in a selected format like .eps. The results of the run can be found on the terminal screen. This included the fit for each PMT, the total stopping muon rate and the total passing muon rate.

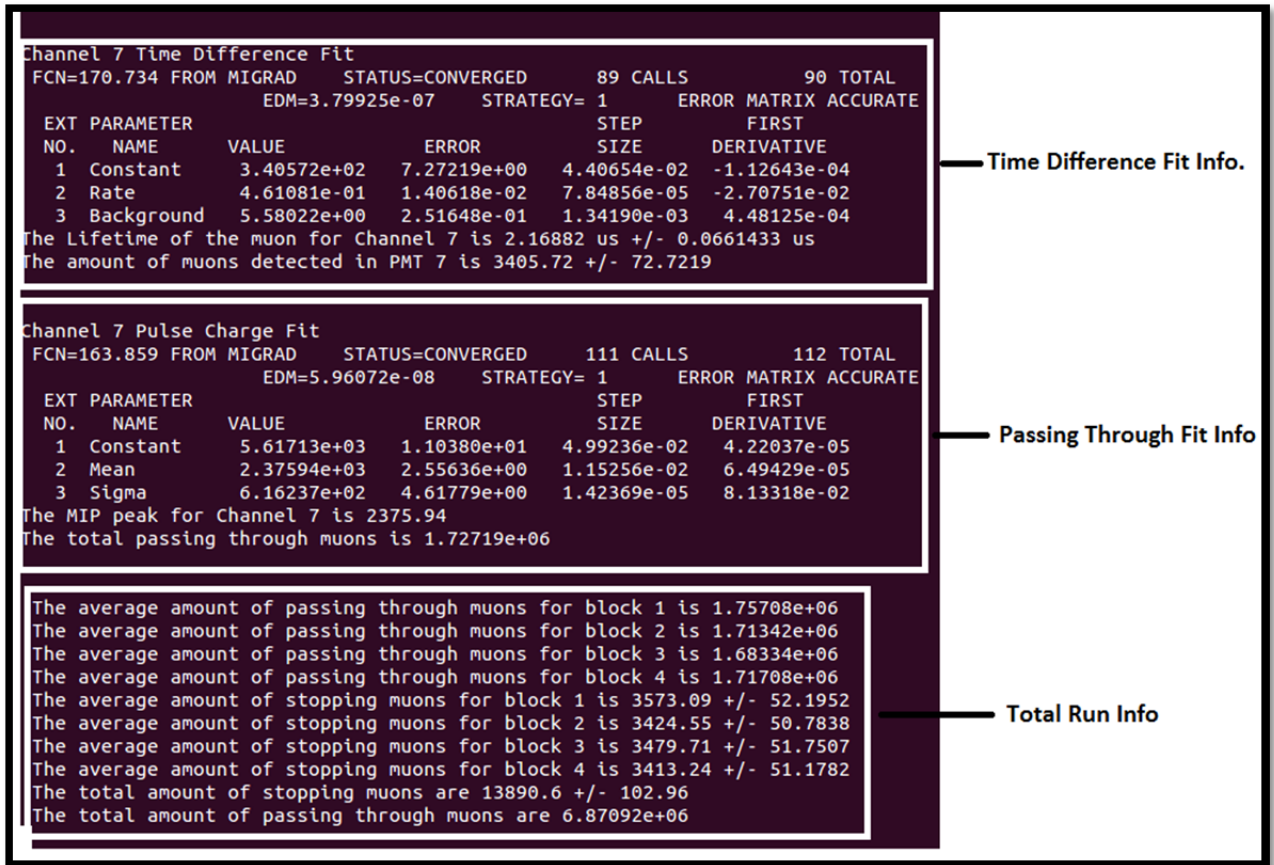


FIG 16: Fit information for PMT

STEP 8: Click the quit button or close the window. (Cntrl c).

STEP 9: Once the analysis window is closed Enter: **emacs previous_run_results.txt**. This will produce a text file with all the results of the previous run. Save this file in Project/smd/analyzer/observations. Using the name convention seen their.

STEP 10: The information can then be entered in the run log found in SMD_run_log.xlsx

Turning off the Detector

Before the detector can be moved it must be properly disassembled.

STEP 1: Turn off the HV by selecting **HV OFF** button. You can see the voltage decrease by selecting the **V6533** link.




FIG 17: V6533 link

STEP 2: Once the voltage is at zero select the programs tab.




FIG 18: Programs tab on the MIDAS control

STEP 3: Click **Stop** on the scV6533 and fev17120psd system. They should turn red.

STEP 4: Turn off the power button, and unplug the power cables. The Detector is now ready to be moved. If possible the laptop can remain connected to V1718 Master Module.



FIG 18: Power Button on CAEN crate

Performing your own Measurements and Analysis

On-line Software/Analyzer

As indicated above, pulses from the eight PMTs attached to the bars are digitized by the CAEN V1720 digitizer card. This card has a 250 MSPS (Mega-sample per second) ADC for each channel. The data from this ADC is processed in real time by the Field Programmable Gate Array (FPGA) on the digitizer card to find and process hits. The online pulse processing that is implemented on this card is called PSD (Pulse Shape Discrimination). The basic idea is that you get a charge and a time for each individual hit that the FPGA finds. The online monitoring can be used to display information from the DAQ during a run. To start the online monitor enter

```
/home/daquser/online/src/analyzer/SmdDisplay.exe
```

The same program can also be used on a MIDAS file that has already been written. For instance,

```
/home/daquser/online/src/analyzer/SmdDisplay.exe /home/daquser/Data/run00016.mid.gz
```

The program shows plots of the charge, time difference between hits and waveforms for each of the digitizer's channels.

Output Data Text Files

Once a run is finished, another program automatically converts the key information in the MIDAS file to a text file. These files can be analyzed by you using whatever program you like e.g. ROOT, Gnuplot, Excel. The text files are in the directory

```
/home/daquser/Data/text_output/
```

The output text file consists of lists of the last 10 SMD hits in each channel, with one hit per line. Each line consists of three numbers:

TimeTag, Channel, Charge

where

- TimeTag: the internal clock time for each hit; clock is 250MHz; multiply TimeTag by 4 to get time in nanoseconds.
- Channel: 0-7, the channel of the 1720 digitizer
- Charge: the integrated charge for the pulse (in digital counts)

To find coincidences between the two ends of bars or between bars, write a program to sort through the list of times to find matches (or near matches). To find double hits (e.g. indicative of muon stop and decay) find time matches within the 20 μs time memory of the digitizers.

Propose and Perform Measurements

The SMD setup is quite versatile, so many possible measurements can be performed and different configurations of the scintillator bars can be made as indicated in fig. 5. Some measurements might involve the use of additional material in which to stop muons or to ensure that you are dealing with high momentum particles. ***Before reconfiguring the scintillators (see fig. 5) consult the lab supervisor and turn off all PMT high voltages.***

Some example measurements relating to the detector performance and the properties of muons are the following:

- Detection efficiency vs. voltage
- Cosmic ray muon dE/dx
- Stopping muon ΔE
- Timing resolution of the PMTs and bars $dT(\Delta E)$ e.g. end-end, between bars, etc.
- Spatial resolution of bars using signals from two ends and/or multiple bars or use $\mu \rightarrow e$ decay; this would be useful in correlating the positions of the through-going and stopping muons, and decay electrons or positrons.
- Positive Muon lifetime
- Lifetime of negative muons stopping in materials; stopping negative muons can form muonic atoms which result in alternate lifetimes which vary considerably depending on the material. ^[6]
- $\mu \rightarrow e$ decay energy measurement (using one or more bars); special and timing information is valuable here.
- μ^-e decay forward-backward asymmetry to determine polarization of positively charged cosmic ray muons; this requires some more subtle considerations since muons depolarize in some materials like plastic scintillator.

Form a small group of 2-4 students and propose a set of measurements using a particular configuration of the four bars; once begun, measurements can be monitored remotely and data can be taken over a 10-24 hour period. Explain briefly how you will perform the proposed measurements and what your expectations are. Discuss your proposal with the lab supervisor or others.

(For Phys. 531: Submit the proposal including some proposed days and times for the measurements (≤ 1 page) to the Phys531 Program Review Committee (DB!).) After taking the data and analyzing it, write up a brief summary of the measurements, results, and comparison with expectations (e.g. simulations, calculations, other known measurements, if any, etc.).

Appendix 1

Moving the detector (unplugged)

The detector rests on top of a pull cart with wheels, this allows it to be moved around. The only requirement of moving the detector is a power outlet. Access to the TRIUMF network is helpful, as it allows you to enter the computer from an external output, but not compulsory for performing a run.

STEP 1: Move the detector to the desired location.

STEP 2: Connect the black and grey plugs to an outlet. The black plug powers the CAEN crate and the Grey plug is for an older system. They usually come out the back of the detector.

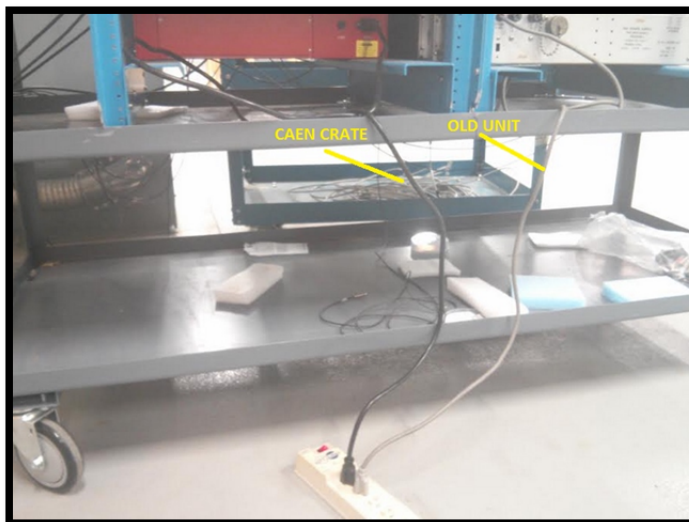


FIG 19: Power cord of the CAEN CRATE and OLD Unit

STEP 3: Reconnect the USB output from the V1718 Master module to the laptop.



FIG 20: V1718 Output USB

STEP 4: Power on the detector by switching the green power button

STEP 5: The detector is turned on by reversing the order of how it was turned off. Make sure the voltages are fully ramped up before starting a run.

Opening A TRIUMF Network Link

On occasions when the detector is moved the connection to the TRIUMF network must be re-established. This also works if the computer is restarted. For this to work the laptop must be connected to a working Ethernet port. The laptop can be run locally through: **localhost:8081** whether or not it is connected to the network.

STEP 1: Make sure the laptop is connected to the internet and open a terminal

STEP 2: Enter: **cd online/src/bin**

STEP 3: Enter: **./start_daq.sh** This will open the connection and if everything is working should produce a MIDAS front end window under the link **daqlap01.triumf.ca:8081**

STEP 4: Once this link is established you will be able to access the laptop from other computer connected to the TRIUMF network.

STEP 5: To do this open a terminal on your own personal computer. Enter: **ssh midas@daqlap01.triumf.ca -X**

STEP 6: You will then be asked for a password. This can be obtained from Pierre Amaudruz or Doug Bryman.

Appendix 2

On-line Analysis Program Details

This section will contain a brief introduction to the code layout of the built-in analysis program. It will also detail auxiliary scripts that have been developed. It will give instructions on how to run this script. Knowledge of C++ and root is required to modify the program.

Introduction to the Analysis Program

The analysis program is collaboration of ten different files. A brief description is given below. The files must be compiled before the analysis program can be run.

TWaveformHisto.cxx: Creates the class that creates the histogram for the wavefunction of the individual pulses. Relevant header (TWaveformHisto.h) is included.

TV1720DppData.cxx: Create a class to store the V1720 Dpp information. Relevant header (TV1720DppData.h) is included.

TV1720WaveformData.cxx: Creates a class to store the V1720 waveforms from the DPP processing. Relevant header (TV1720WaveformData.h) is included.

SmdDisplay.cxx: This is the main function and create the GUI for the analysis program. Relevant header (SmdDisplay.h) is included.

TSmdAnaManager.cxx: This class fills the different histograms. Also includes the option to output the data to: **Projects/smd/analyzer/compcoinc**. See below for more information. Relevant header (TV1720WaveformData.h) is included.

TDppPulseChargeHisto.h: Creates the histogram for the Passing through muons.

TDppTimeDiffHisto.h: Creates the histogram for the decay time spectrum.

TDppStopMuonEng.h: Creates the histogram for the energy of the stopping muons.

TDppSopElecEng.h: Creates the histogram for the energy of the decay electrons.

Makefile: The make file required for compilation.

Extra Analysis Programs

There are certain results that can only be obtained by running external scripts on the data obtained from a given run. It is not that these scripts couldn't be contained in the analysis program it's that the live event processing would be drastically slowed down by these scripts.

The script is designed to check coincidence between different PMT's. It is currently set up to check muons that pass through three PMT's and stop in a fourth. The energy spectrum of these muons at each step of the way is produced. It can be modified for different functions.

Run the Program

STEP 1: Choose the run you would like to check the coincidence of. (ex 356 or something) and open a terminal.

STEP 2: Enter: **cd online/src/analyzer**. When the selected run is analyzed you need the data to be saved in external text files. In this way more complicated analysis can be performed.

STEP 3: The analysis program already contains the code necessary to output the data as external text files it is just commented out. The analysis program runs faster when text output section is commented out. Enter: **emacs TSmdAnaManager.h &**

STEP 4: Un-comment the following section. Then save and close the file.

" data-bbox="172 407 941 697"/>

```
emacs@lpdaq02
File Edit Options Buffers Tools C Help

// Array of DPP pulse charges
TDppPulseChargeHisto *DppPulseChargeHisto;
TDppTimeDiffHisto *DppTimeDiffHisto;
TDppStopMuonEngHisto *DppStopMuonEngHisto;
TDppStopElecEngHisto *DppStopElecEngHisto;
TWaveformsHisto *WaveformsHisto;

//Outfiles contain the relevant data for more complex analysis without incorporating it directly into the Smd_Analyzer
//The files are saved in the results directory
/*ofstream outfile0C;
ofstream outfile0T;
ofstream outfile1C;
ofstream outfile1T;
ofstream outfile2C;
ofstream outfile2T;
ofstream outfile3C;
ofstream outfile3T;
ofstream outfile4C;
ofstream outfile4T;
ofstream outfile5C;
ofstream outfile5T;
ofstream outfile6C;
ofstream outfile6T;
ofstream outfile7C;
ofstream outfile7T;
*/
```

FIG 22: Section required to un-comment on the TSmdAnaManager.h file

STEP 5: Enter: **emacs TSmdAnaManager.cxx &**. Un-comment the following two section. Then save and close the file

' and \"/'". The Emacs window title is 'emacs@lpdaq02' and the menu bar includes 'File Edit Options Buffers Tools C++ Help'."/>

```
emcs@lpdaq02
File Edit Options Buffers Tools C++ Help

DppStopMuonEngHisto = new TDppStopMuonEngHisto();
DppStopMuonEngHisto->DisableAutoUpdate();

DppStopElecEngHisto = new TDppStopElecEngHisto();
DppStopElecEngHisto->DisableAutoUpdate();

WaveformsHisto = new TWaveformsHisto();
WaveformsHisto->DisableAutoUpdate();

/*
outfile0C.open("/home/midas/Projects/smd/analyzer/compcoinc/results0C.txt");
outfile0T.open("/home/midas/Projects/smd/analyzer/compcoinc/results0T.txt");
outfile1C.open("/home/midas/Projects/smd/analyzer/compcoinc/results1C.txt");
outfile1T.open("/home/midas/Projects/smd/analyzer/compcoinc/results1T.txt");
outfile2C.open("/home/midas/Projects/smd/analyzer/compcoinc/results2C.txt");
outfile2T.open("/home/midas/Projects/smd/analyzer/compcoinc/results2T.txt");
outfile3C.open("/home/midas/Projects/smd/analyzer/compcoinc/results3C.txt");
outfile3T.open("/home/midas/Projects/smd/analyzer/compcoinc/results3T.txt");
outfile4C.open("/home/midas/Projects/smd/analyzer/compcoinc/results4C.txt");
outfile4T.open("/home/midas/Projects/smd/analyzer/compcoinc/results4T.txt");
outfile5C.open("/home/midas/Projects/smd/analyzer/compcoinc/results5C.txt");
outfile5T.open("/home/midas/Projects/smd/analyzer/compcoinc/results5T.txt");
outfile6C.open("/home/midas/Projects/smd/analyzer/compcoinc/results6C.txt");
outfile6T.open("/home/midas/Projects/smd/analyzer/compcoinc/results6T.txt");
outfile7C.open("/home/midas/Projects/smd/analyzer/compcoinc/results7C.txt");
outfile7T.open("/home/midas/Projects/smd/analyzer/compcoinc/results7T.txt");
*/
```

FIG 24: First section required to un-comment on the TSmdAnaManager.cxx file

' and \"/'". The Emacs window title is 'emacs@lpdaq02' and the menu bar includes 'File Edit Options Buffers Tools C++ Help'."/>

```
emcs@lpdaq02
File Edit Options Buffers Tools C++ Help

<< pulse->Pur << std::endl;
DppPulseChargeHisto->GetHistogram(pulse->Channel)->Fill(pulse->ChargeShort);
//Output file section////////////////////////////////////
/* if(pulse->Channel == 0){
outfile0C << pulse->ChargeShort<<endl;
outfile0T << pulse->TimeTag<<endl;
}

if(pulse->Channel == 1){
outfile1C << pulse->ChargeShort<<endl;
outfile1T << pulse->TimeTag<<endl;
}
if (pulse->Channel == 2){
outfile2C << pulse->ChargeShort<<endl;
outfile2T << pulse->TimeTag<<endl;
}
if (pulse->Channel == 3){
outfile3C << pulse->ChargeShort<<endl;
outfile3T << pulse->TimeTag<<endl;
}
if (pulse->Channel == 4){
outfile4C << pulse->ChargeShort<<endl;
outfile4T << pulse->TimeTag<<endl;
}
if (pulse->Channel == 5){
outfile5C << pulse->ChargeShort<<endl;
outfile5T << pulse->TimeTag<<endl;
}
if (pulse->Channel == 6){
outfile6C << pulse->ChargeShort<<endl;
outfile6T << pulse->TimeTag<<endl;
}
if (pulse->Channel ==7){
outfile7C << pulse->ChargeShort<< endl;
outfile7T << pulse->TimeTag<< endl;
}*/
////////////////////////////////////
```

FIG 25: Second section required to un-comment on the TSmdAnaManager.cxx file

STEP 6: Because changes have been made the analyzer needs to be re-compiled. Enter: **make clean**. Then Enter: **make**. This will compile the analyzer

STEP 7: Run the desired run (See Running an analysis on a previous run). The data from the PMT's will be put into external text files. The text files are located in the directory **/home/daquser/Data/compcoinc**. Each PMT has 2 files.

- 1) results#C.txt: This contains the energy of each pulse from the PMT #
- 2) results#T.txt: This contains the time tag of each pulse from the PMT #

NOTE: If you run another analysis the text files will get overwritten by the values of that case. So once you're finished you should comment out the output section and recompile.

STEP 8: Close the analysis window and Enter: **cd compcoinc**.

STEP 9: Enter: **emacs fourcoinc.C &**. This file is the script that performs the coincidence analysis. The code is designed to look for muons that stop in PMT 1, it then will determine what other PMT this muon travelled through. Currently it is set up to check PMT 3, 5 and 7 (one from each block). It can be configured to your personnel needs.

STEP 10: Before the script can be started the number of events from the text files must be entered. The number of events can be taken from the event files themselves. Just Enter: **emacs results#C.txt &**. Scroll to the very end and look at the line number. This must be done for all PMT's.


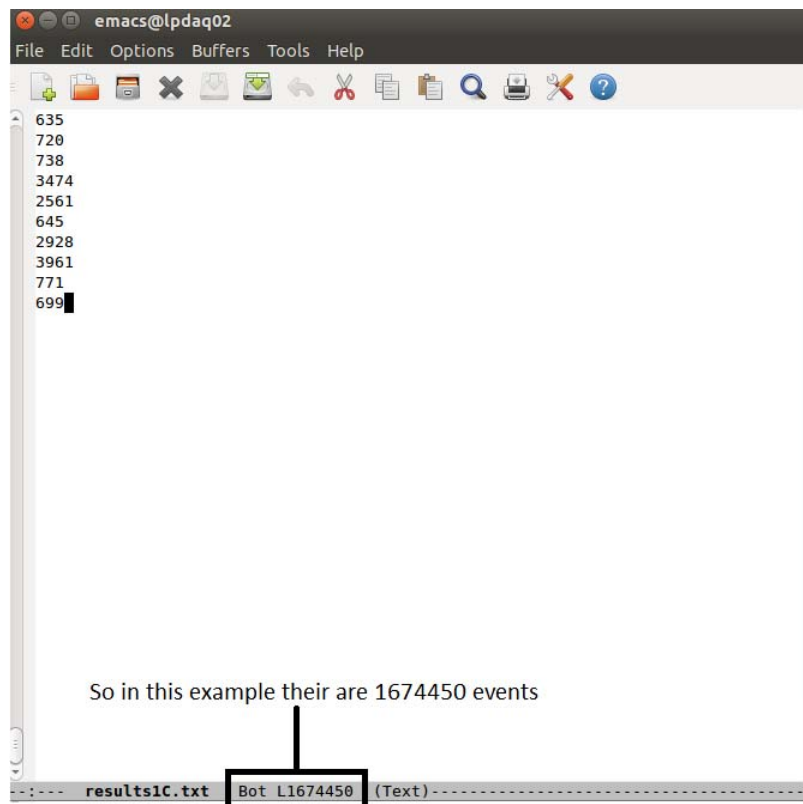


FIG 26: Number of event files for PMT 1

STEP 11: The event must be entered for each PMT. The section that they must be entered in is highlighted here.

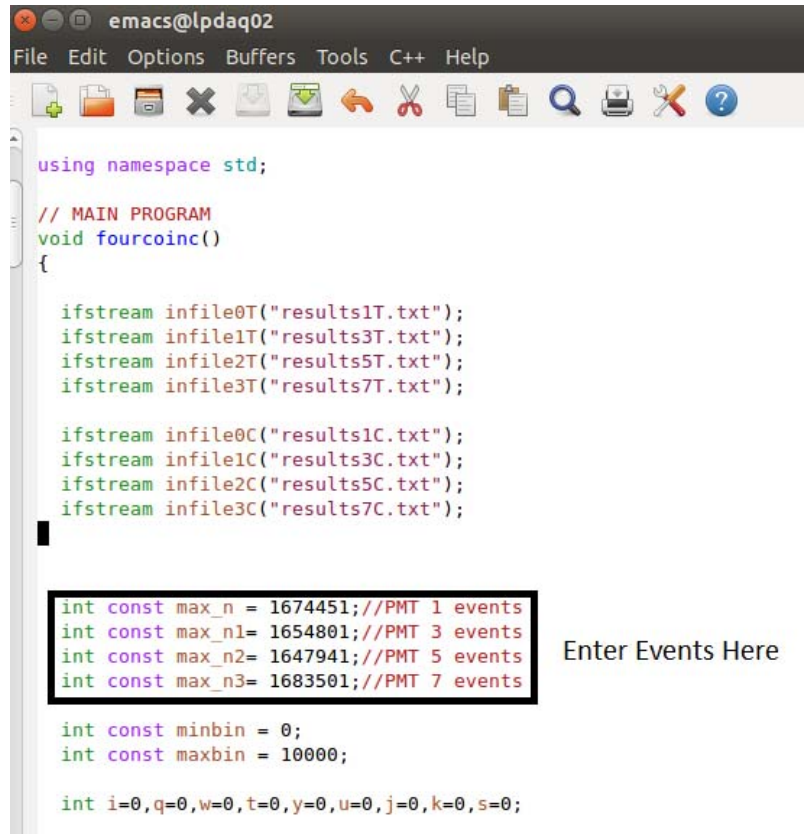

```
emacs@lpdaq02
File Edit Options Buffers Tools C++ Help

using namespace std;

// MAIN PROGRAM
void fourcoinc()
{

    ifstream infile0T("results1T.txt");
    ifstream infile1T("results3T.txt");
    ifstream infile2T("results5T.txt");
    ifstream infile3T("results7T.txt");

    ifstream infile0C("results1C.txt");
    ifstream infile1C("results3C.txt");
    ifstream infile2C("results5C.txt");
    ifstream infile3C("results7C.txt");

    int const max_n = 1674451; //PMT 1 events
    int const max_n1= 1654801; //PMT 3 events
    int const max_n2= 1647941; //PMT 5 events
    int const max_n3= 1683501; //PMT 7 events

    int const minbin = 0;
    int const maxbin = 10000;

    int i=0,q=0,w=0,t=0,y=0,u=0,j=0,k=0,s=0;
```

Enter Events Here

FIG 27: Enter the events

STEP 12: Once the events are properly entered save the document then close it.

STEP 13: Enter: **root -l**

STEP 14: Enter: **.x fourcoinc.C**. This will start the run.

STEP 15: The run will go for a while, when it is finished it will produce the following in the terminal. This will show the percent of muons that passed through each PMT.

Appendix 3

Signal and HV Cabling

Light Guide Label	Signal cable	Digitizer Channel Caen 1720	PMT HV Cable SMVHV	HV Power Supply Caen 6533 Channel	Nominal HV(V)
1a	Spare B	0	5	1	1644
1b	SMD 1	1	2	4	1663
2a	SMD2	2	7	4	1663
2b	SMD3	3	1	0	1693
3a	SMD4	4	6	5	1584
3b	SMD5	5	3	2	1680
4a	Spare A	6	4	Fluke	1650
4b	SMD7	7	8	3	1550

Acknowledgments

The original author would like to thank Ewart Blackmore and Mike Trinczek for all their help and support. The Phys. 531/GRIDS-TSI crew would like to thank Pierre Amadruz and Thomas Lindner for developing and assistance with the detector software.



FIG 21: Ewart Blackmore who built the SMD Detector.

References

- 1) E. Blackmore et al., IEEE Trans. Nuc. Sci. 62,2792 (2015).
- 2) Matthew Stukel; Carleton University; *PHYS 3007: Laboratory #4: Muon Lifetime*
- 3) CAEN; Technical Information Manual; VME Programmable HV Power Supply
- 4) CAEN; Technical Information Manual; MOD V1720 Digitizer; CAEN; UM 2580 DPSD User Manual
- 5) CAEN; Technical Information Manual; MOD V178 Master Controller
- 6) T.Suzuki and D.F. Measday; UBC; Total nuclear capture rates for negative muons